




Biodesign™

SURGISIS® ANTERIOR PELVIC FLOOR GRAFT

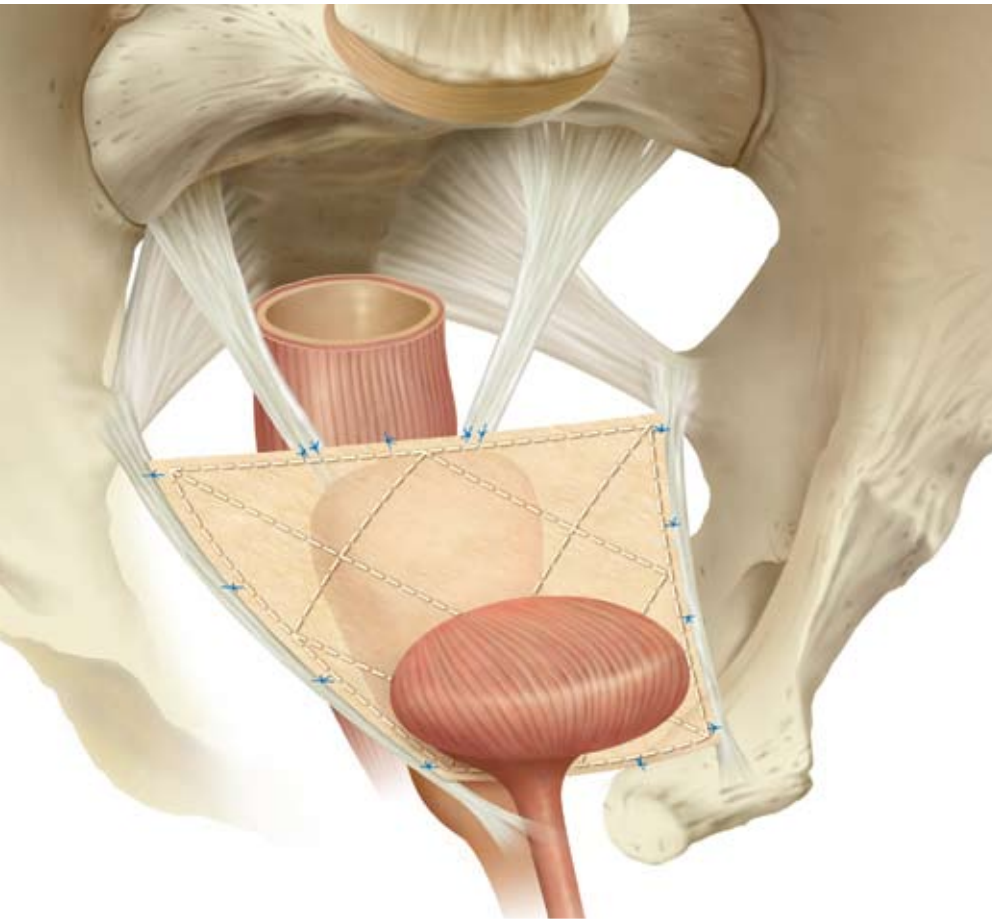

Restore a pelvic floor, and a way of life.


For centuries women have suffered the discomfort and embarrassment of pelvic organ prolapse, often in silence. Today, women desire a quality of life that allows them to continue enjoying their daily activities.

Biodesign enables you to restore your patient's quality of life. Biodesign communicates with the body, signaling surrounding cells to grow across the scaffold. The result? Completely remodeled, vascularized tissue that's strong yet flexible. And unlike synthetic mesh and cross-linked biologic grafts, it is resistant to infection, encapsulation and erosion into surrounding tissue.

Biodesign is remarkably simple to handle and can easily be trimmed to any shape or size.

Cook Medical—Improving quality of life for patients through advanced tissue repair.

Global Product Number	Order Number	Size cm
Anterior Pelvic Floor Graft		
G46605	J-PF-ANT	9 x 12
4-Layer Tissue Graft		
G18941	J-SLH-4S-4X7	4 x 7
G18681	J-SLH-4S-7X10	7 x 10
G18682	J-SLH-4S-7X20	7 x 20
G46612	J-PF-8X13	8 x 13
G48667	J-PF-10X15	10 x 15
G52412	J-PFV-4X7	4 x 7 (perforated)
G46604	J-PFV-9X14	9 x 14 (perforated)

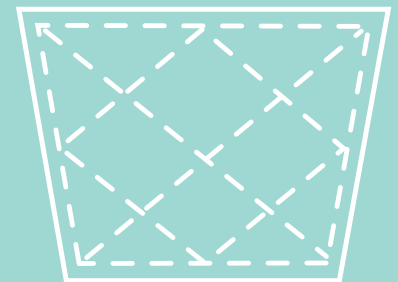

Anterior Pelvic Floor Graft



4-Layer Tissue Graft

FEATURES & BENEFITS

- Easy to hydrate and suture.
- Minimal scarring.
- Migration and erosion resistant.
- Does not encapsulate.
- Restores natural form and function.

TIPS

- When sizing Biodesign, be sure to **trim a large enough piece for the defect**. Too small a piece may create tension on sutures and cause recurrence.
- Use only antiseptics and antimicrobials that have proven compatible with wound healing. Problems have been reported with gentamicin, povidone iodine, bacitracin, polymyxin B and vancomycin.
- Slow-resorbing or nonabsorbable sutures are recommended.
- After surgery, patients should abstain from heavy lifting, strenuous exercise and sexual intercourse for 4 to 6 weeks.

DATA

1. Arunkalaivanan A. Pelvic floor reconstruction using Surgisis (porcine mesh) graft. Poster presented at: Joint Meeting of the International Continence Society and the International Urogynecological Association 34th Annual Meeting; August 25-27, 2004; Paris, France.
2. Chaliha C, Khalid U, Campagna L, et al. SIS graft for anterior vaginal wall prolapse repair—a case-controlled study. *Int Urogynecol J Pelvic Floor Dysfunct.* 2006;17(5):492-497.
3. Cutner A, Spiteri M, Osborne J. Use of absorbable mesh to prevent posterior vaginal wall prolapse after laparoscopic sacrocolpopexy. *Int Urogynecol J Pelvic Floor Dysfunct.* 2001;12:577.
4. Franklin ME Jr, Treviño JM, Portillo G, et al. The use of porcine small intestinal submucosa as a prosthetic material for laparoscopic hernia repair in infected and potentially contaminated fields: long-term follow-up. *Surg Endosc.* 2008;22(9):1941-1946.
5. Hiles M, Hodde J. Tissue engineering a clinically useful extracellular matrix biomaterial. *Int Urogynecol J Pelvic Floor Dysfunct.* 2006;17(suppl 1):S39-S43.
6. Reid RI, Hodde J. The histological pattern of xenograft remodeling in vaginal paravaginal repair with Surgisis overlay graft. *Int Urogynecol J Pelvic Floor Dysfunct.* 2006;17(suppl 2):S120. Abstract 105.
7. Reid, RI. A retrospective analysis of recto-enterocele repair with Surgisis biomesh. Poster presented at: 31st Annual Meeting of the International Urogynecological Association; September 6-9, 2006; Athens, Greece.
8. Reid RI. A retrospective analysis of vaginal paravaginal repair with Surgisis for severe cysto-urethrocele. Poster presented at: 31st Annual Meeting of the International Urogynecological Association; September 6-9, 2006; Athens, Greece.
9. Ross JW. Pelvic floor hernias: tissue repair or replacement? *Laparoscopy Today* Web site. 2003. http://www.laparoscopytoday.com/2003/01/pelvic_floor_he.html. Accessed March 13, 2009.
10. Rutner AB, Levine SR, Schmaelzle JF. Processed porcine small intestine submucosa as a graft material for pubovaginal slings: durability and results. *Urology.* 2003;62(5):805-809.
11. Sardeli C, Axelsen SM, Bek KM. Use of porcine small intestinal submucosa in the surgical treatment of recurrent rectocele in a patient with Ehlers-Danlos syndrome type III. *Int Urogynecol J Pelvic Floor Dysfunct.* 2005;16(6):504-505.
12. Sardeli C, Bek KM, Axelsen SM. Use of porcine small intestinal submucosa mesh in the surgical treatment of recurrent pelvic organ prolapse. Poster presented at: International Continence Society 35th Annual Meeting; August 28-September 2, 2005; Montreal, Canada.
13. Sung VW, Sokol ER, Rardin CR, et al. Porcine-derived small intestinal submucosa graft-augmented rectocele repair. *J Pelvic Med Surg.* 2004;10(suppl 1):S67. Poster 124.
14. Trabuco EC, Klingele CJ, Gebhart JB. Xenograft use in reconstructive pelvic surgery: a review of the literature. *Int Urogynecol J Pelvic Floor Dysfunct.* 2007;18(5):555-563.
15. Turner RJ, Stanford EJ, Voet RL, et al. Histologic findings of porcine intestinal allograft at 2-4 years after implantation. Poster presented at: AAGL 34th Annual Meeting; November 9-12, 2005; Chicago, IL.

PROCEDURAL AREAS

HERNIA REPAIR
FISTULA REPAIR
PLASTIC & RECONSTRUCTIVE/ENT
STAPLE LINE REINFORCEMENT
PEYRONIE'S REPAIR
CONTINENCE RESTORATION
DURAL REPAIR
PELVIC FLOOR REPAIR

ANTERIOR
ANTERIOR PELVIC FLOOR GRAFT
4-LAYER TISSUE GRAFT
POSTERIOR

EVOLUTION OF TISSUE REPAIR



Biodesign is a breakthrough technology that provides signals and support for the body to restore itself. It incorporates the best attributes of a biologic graft—complete remodeling and resistance to infection—yet it is easy to use, widely available and moderately priced.



www.cookmedical.com

COOK MEDICAL INCORPORATED

P.O. Box 4195, Bloomington, IN 47402-4195 U.S.A.
Phone: 812.339.2235, Toll Free: 800.457.4500, Toll Free Fax: 800.554.8335

COOK (CANADA) INC.

111 Sandiford Drive, Stouffville, Ontario, L4A 7X5 CANADA
Phone: 905.640.7110, Toll Free: 800.668.0300

WILLIAM A. COOK AUSTRALIA PTY. LTD.

95 Brandl Street, Brisbane Technology Park, Eight Mile Plains
Brisbane, QLD 4113 AUSTRALIA, Phone: +61 7 3841 1188

COOK IRELAND LTD.

O'Halloran Road, National Technology Park, Limerick, IRELAND
Phone: 353 613 34440

© COOK 2009 SUR-BM-PFLA-EN-200904

AORTIC
INTERVENTION

CARDIOLOGY

CRITICAL
CARE

ENDOSCOPY

INTERVENTIONAL
RADIOLOGY

PERIPHERAL
INTERVENTION

SURGERY

UROLOGY

WOMEN'S
HEALTH