


Hiatal hernia reinforcement associated with a **LOW RISK OF EROSION**¹


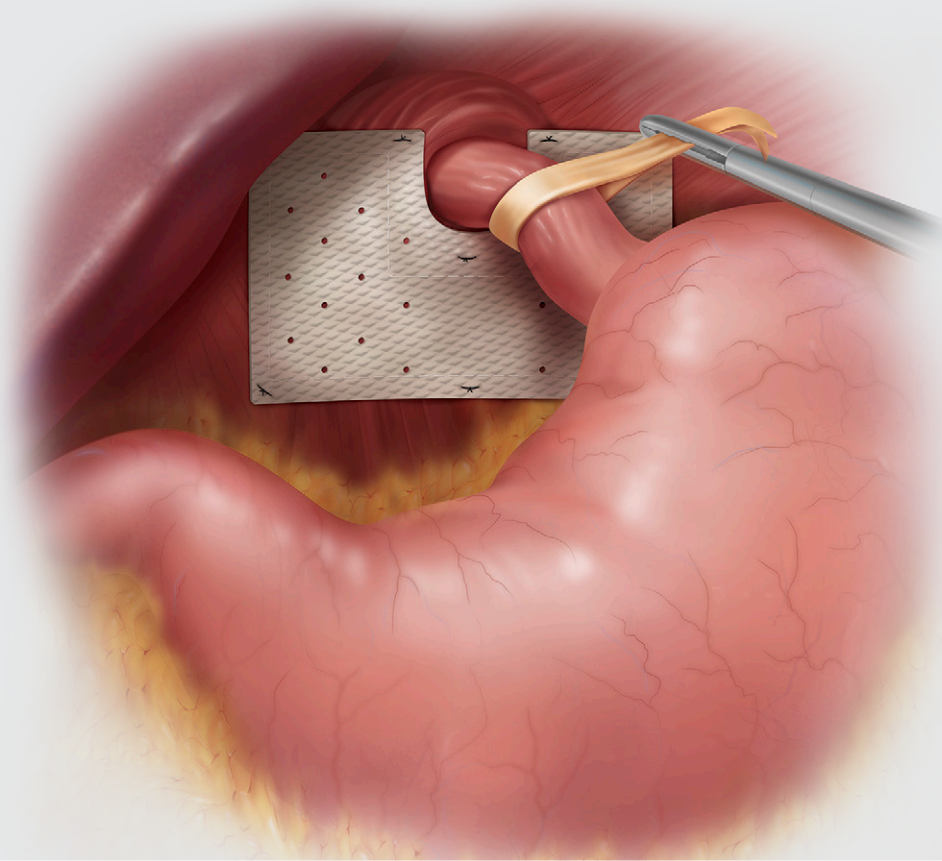


Illustrations by Lisa Clark

Biodesign[®]
ADVANCED TISSUE REPAIR

A surgeon saw a need. We listened. Biodesign Hiatal Hernia Graft is made from a biologic technology that provides support as it is completely remodeled into patient tissue.²

This biologic graft, an extracellular matrix, doesn't contain a meaningful amount of elastin.³ Plus, new blood vessels can grow into the open, three-dimensional structure of the matrix.⁴

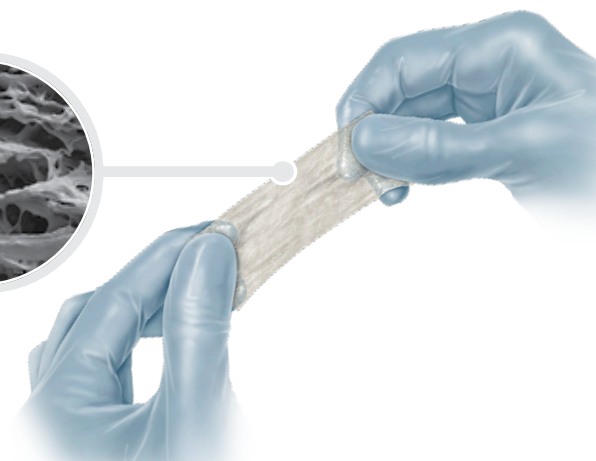

COOK[®]
MEDICAL



BIODESIGN HIATAL HERNIA GRAFT

Used for implantation to reinforce soft tissue where weakness exists, including repair of hiatal hernias.

- The Biodesign Hiatal Hernia Graft is associated with low rates of erosion.¹
- Small intestinal submucosa (SIS), the biomaterial used in the Biodesign Hernia Graft, remodels into patient tissue.²
- SIS is an extracellular matrix that doesn't contain a meaningful amount of elastin.³
- New blood vessels can grow into the open structure of the matrix.²

Order Number	Reference Part Number	Size cm	Comments
G31455	C-PHR-7X10-U	7 x 10	Preshaped
G23947	C-PHR-7X10-AP	7 x 10	Preshaped
G51578	C-PHR-7X10	7 x 10	Standard

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

1. Oelschläger BK, Pellegrini CA, Hunter JG, et al. Biologic prosthesis to prevent recurrence after laparoscopic paraesophageal hernia repair: long-term follow-up from a multicenter, prospective, randomized trial. *J Am Coll Surg.* 2011;213(4):461-468.
2. Nihsen ES, Johnson CE, Hiles MC. Bioactivity of small intestinal submucosa and oxidized regenerated cellulose/collagen. *Adv Skin Wound Care.* 2008;21(10):479-486.
3. Heise RL, Ivanova J, Parekh A, et al. Generating elastin-rich small intestinal submucosa-based smooth muscle constructs utilizing exogenous growth factors and cyclic mechanical stimulation. *Tissue Eng Part A.* 2009;15(12):3951-3960.

Customer Service

EU Website: cookmedical.eu
 EDI: cookmedical.eu/edi
 Distributors: +353 61239240, ssc.distributors@cookmedical.com
 Austria: +43 179567121, oe.orders@cookmedical.com
 Belgium: +32 27001702, be.orders@cookmedical.com
 Denmark: +45 38487607, da.orders@cookmedical.com
 Finland: +358 972519996, fi.orders@cookmedical.com
 France: +33 171230269, fr.orders@cookmedical.com
 Germany: +49 6950072804, de.orders@cookmedical.com
 Hungary: +36 17779199, hu.orders@cookmedical.com
 Iceland: +354 800 7615, is.orders@cookmedical.com
 Ireland: +353 61239252, ie.orders@cookmedical.com
 Italy: +39 0269682853, it.orders@cookmedical.com
 Netherlands: +31 202013367, nl.orders@cookmedical.com
 Norway: +47 23162968, no.orders@cookmedical.com
 Spain: +34 912702691, es.orders@cookmedical.com
 Sweden: +46 858769468, se.orders@cookmedical.com
 Switzerland - French: +41 448009609, fr.orders@cookmedical.com
 Switzerland - Italian: +41 448009609, it.orders@cookmedical.com
 Switzerland - German: +41 448009609, de.orders@cookmedical.com
 United Kingdom: +44 2073654183, uk.orders@cookmedical.com

USA Website: cookmedical.com

EDI: cookmedical.com/edi.do

Americas:

Phone: +1 812.339.2235, 800.457.4500, Fax: 800.554.8335

E-mail: orders@cookmedical.com

Australia:

Phone: +61 734346000, 1800777222, Fax: +61 734346001, 1800077283

E-mail: cau.custserv@cookmedical.com



AI-ESC-IR-OHNS-PI-RH-SUR-A4